

COMPANY PROFILE



GREAT LABORATORY & CHEMICAL SUPPLIERS LTD



www.greatlab.co.ke

INTRODUCTION

Founded in 2015, Great Laboratory and Chemical Suppliers Ltd, is a reputable supplier of high-quality medical products and laboratory consumables. With a commitment to excellence, we specialize in supplying a comprehensive range of medical and laboratory essentials tailored to meet the needs of healthcare institutions, laboratories, and research facilities.

Our product portfolio includes, but not limited to:

- **Surgical items**
- **Dressings and sutures**
- **Dental items**
- **Medical equipment**
- **Laboratory consumables**

We pride ourselves on offering top-tier products sourced from trusted manufacturers, ensuring that your institution receives only the best in terms of quality, reliability, and cost-effectiveness. Our products are competitively priced, and we offer prompt and efficient delivery services to meet your organization's needs.

MISSION

Our mission is lived everyday by providing our clients with the highest quality products to improve patient care in Kenya and Africa.

VISION

To be the trusted provider of high- quality, innovative and affordable medical supplies delivering exception customer service to foster healthier communities.



Disposal Circular Stapler

Three - Row - Staple Type





| NO. | Specification | Staple bin color | ΦD(mm) | Diameter of cutter knife Φ d (mm) | Staple quantity | Staple specification Φ d1*h (mm) |
|-----|---------------|------------------|--------|--------------------------------------|-----------------|-------------------------------------|
| 1 | SRDGX-B-24 | White | Φ25.5 | Φ14.6 | 30 | 0.3*4.6/4.6/4.8 |
| 2 | SRDGX-B-26 | Yellow | Φ27.5 | Φ16.4 | 36 | 0.3*4.8/5.0/5.2 |
| 3 | SRDGX-B-29 | Purple | Φ30.5 | Φ20 | 36 | 0.3*4.8/5.0/5.2 |
| 4 | SRDGX-B-32 | Black | Φ32.7 | Φ22 | 45 | 0.3*4.8/5.0/5.2 |

Disposal Linear Cutter Stapler



| NO. | Specification | Suturing length (mm) | Cutting length (mm) | Staple quantity | Staple specification (mm) |
|-----|---------------|-------------------------|------------------------|-----------------|------------------------------|
| 1 | SRDLC-A60B | 65±2 | 60 | 64 | 0.2*3.8 |
| 2 | SRDLC-A60G | 65±2 | 60 | 64 | 0.2*4.8 |
| 3 | SRDLC-A80B | 85±2 | 80 | 84 | 0.2*3.8 |
| 4 | SRDLC-A80G | 85±2 | 80 | 84 | 0.2*4.8 |
| 5 | SRDLC-A100B | 101±2 | 100 | 100 | 0.2*3.8 |
| 6 | SRDLC-A100G | 101±2 | 100 | 100 | 0.2*4.8 |
| 7 | SRDLC-B60B | 61±2 | 60 | 60 | 0.2*3.8 |
| 8 | SRDLC-B60G | 61±2 | 60 | 60 | 0.2*4.8 |
| 9 | SRDLC-B80B | 81±2 | 80 | 80 | 0.2*3.8 |
| 10 | SRDLC-B80G | 81±2 | 80 | 80 | 0.2*4.8 |
| 11 | SRDLC-B100B | 101±2 | 100 | 100 | 0.2*3.8 |
| 12 | SRDLC-B100G | 101±2 | 100 | 100 | 0.2*4.8 |

Disposable Linear Cutter Stapler And Reloads

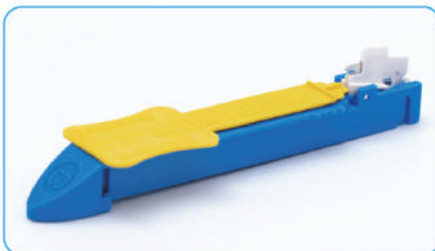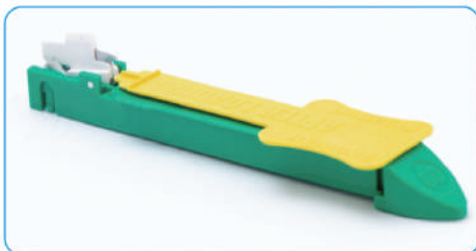

| NO. | Specification | Color | Staple quantity | Staple specification (mm) |
|-----|---------------|-------|-----------------|---------------------------|
| 1 | SRDLC-A60B | Blue | 64 | 0.2*3.8 |
| 2 | SRDLC-A60G | Gold | 64 | 0.2*4.8 |
| 3 | SRDLC-A80B | Blue | 84 | 0.2*3.8 |
| 4 | SRDLC-A80G | Gold | 84 | 0.2*4.8 |
| 5 | SRDLC-A100B | Blue | 100 | 0.2*3.8 |
| 6 | SRDLC-A100G | Gold | 100 | 0.2*4.8 |
| 7 | SRDLC-B60B | Blue | 60 | 0.2*3.8 |
| 8 | SRDLC-B60G | Gold | 60 | 0.2*4.8 |
| 9 | SRDLC-B80B | Blue | 80 | 0.2*3.8 |
| 10 | SRDLC-B80G | Gold | 80 | 0.2*4.8 |
| 11 | SRDLC-B100B | Blue | 100 | 0.2*3.8 |
| 12 | SRDLC-B100G | Gold | 100 | 0.2*4.8 |

Disposable Ligasure



| NO. | Scissor type specification | Jaw angle | Shaft rotation | Shaft diameter (mm) | Shaft length L (cm) | Seal plate Length L (mm) | Cutting length (mm) |
|-----|----------------------------|------------|----------------|---------------------|---------------------|--------------------------|---------------------|
| 1 | SRLS-0520 | Elbow | 350° | 5 | 20 | 20.9 | 19 |
| 2 | SRLS-0823 | Elbow | 350° | 5 | 23 | 20.9 | 19 |
| 3 | SRLS-5120S | Straighter | 350° | 5 | 20 | 16 | 14 |
| 4 | SRLS-1120S | Straighter | 350° | 10 | 20 | 22 | 20 |

| NO. | Handle type specification | Jaw angle | Shaft rotation | Shaft diameter (mm) | Shaft length L (cm) | Seal plate Length L (mm) | Cutting length (mm) |
|-----|---------------------------|------------|----------------|---------------------|---------------------|--------------------------|---------------------|
| 1 | SRLS-0537 | Elbow | 350° | 5 | 37 | 20.9 | 19 |
| 2 | SRLS-0837 | Elbow | 350° | 5 | 37 | 20.9 | 19 |
| 3 | SRLS-5137S | Straighter | 350° | 5 | 37 | 16 | 14 |
| 4 | SRLS-1137S | Straighter | 350° | 10 | 37 | 22 | 20 |



PPH Hemorrhoidal Circular Stapler



Application:

It is suitable for the procedure for prolapse and hemorrhoids.

Features and Advantages:

The design of uniform nail holder (nail anvil) improves the force strength of the nail to ensure the stable and complete molding of the nail.

The large capacity of the nail storage can provide more space for the organization.


The butterfly tail makes it easy for the doctor to exert enough pressure on the tissue.

Firing device to avoid misfiring.

High hardness stainless steel ring knife.

Clear indication needle window design, so that the doctor at any time to grasp the position of the nail site.

Disposable Skin Stapler and Remover



Application:

Used for wound closure and tissue suture

Features and Advantages:

Single use, avoid cross-infection


Biologically compatible

Significantly decrease wound closure time and reduce procedure & anesthesia time

Suture easily and efficiently as well as easily removed

With better cosmetic results

DISPOSABLE LAPERASCOPIC TROCARS

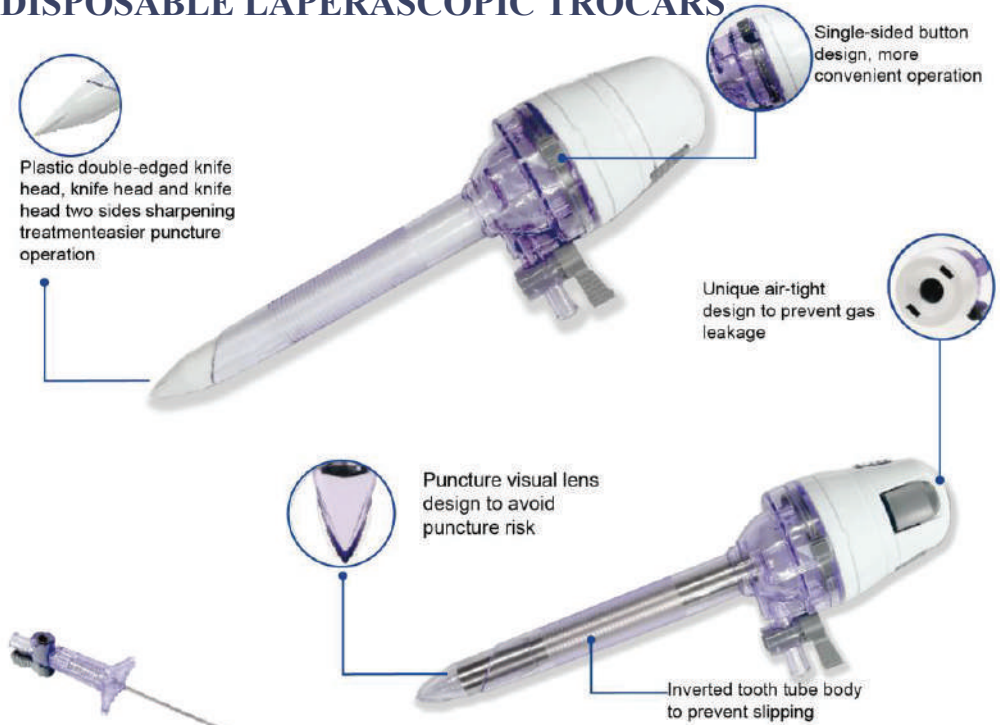


Application:

It is used for laparoscopy surgery, the puncture of the abdominal wall of the human body is used to establish a working channel for abdominal surgery.

DISPOSABLE UNDER PAD



HERNIA REPAIR MESH

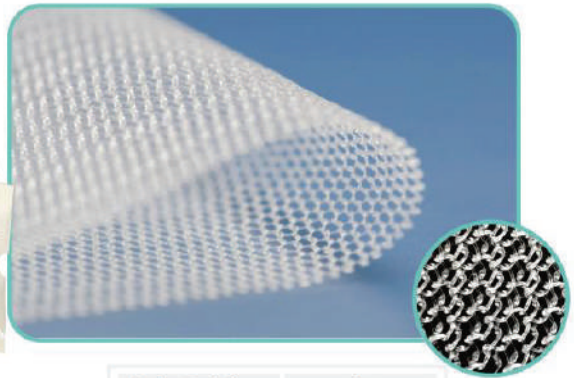

Large mesh aperture

Promotes liquid circulation and smoothes tissue growth.

Less micropores

Greatly reduces the possibility of bacteria hiding and is not easy to infect.


Light weight

Reduce postoperative pain and foreign body sensation.

| Products Description | Size |
|----------------------|----------|
| Polypropylene Mesh | 6x11cm |
| Polypropylene Mesh | 7.6x15cm |
| Polypropylene Mesh | 10x15cm |
| Polypropylene Mesh | 15x15cm |
| Polypropylene Mesh | 15x20cm |
| Polypropylene Mesh | 20x25cm |
| Polypropylene Mesh | 25x25cm |
| Polypropylene Mesh | 25x30cm |
| Polypropylene Mesh | 30x30cm |

CLOSED SUCTION CATHETER

Suction Control Switch
Ergonomic suction control switch with a built-in security lock to visually determine if the device is in the OFF/ON position. Offers a quick and easy, single handed operation design, which allows you to keep your eye on the patient and do no harm. One handed operation allows the free hand to support the ET or Trach device to ensure less trauma to the site.

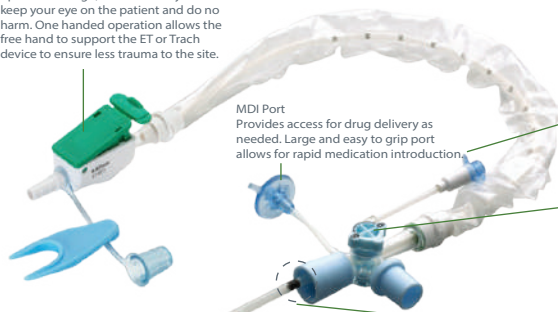

Catheter Tip
Atraumatic rounded catheter tip for minimal tracheal wall injury.

MDI Port
Provides access for drug delivery as needed. Large and easy to grip port allows for rapid medication introduction.

Irrigation Port
Offers a one-way valve to prevent backflow leakage and easy access for cleaning the closed suction system.

Isolation Valve
Seals the irrigation chamber to provide a better cleaning of the catheter. Allows for continuous ventilation and prevents backflow of saline during cleaning to ensure patient comfort and safety.


Black Ring Indicator
Ensures that the catheter is properly withdrawn from the ET or Trach device. Black ring must be visible in the plastic sheath after suctioning the patient.



BIOPSY NEEDLES

AUTOMATIC BIOPSY SYSTEM NEEDLE


- Loading indicator
- Automatic sampling
- Echo-enhancement
- Trigger site on the rear
- Light-weight design & Easy operate
- One bottom for taking samples
- High velocity throw and strong strength

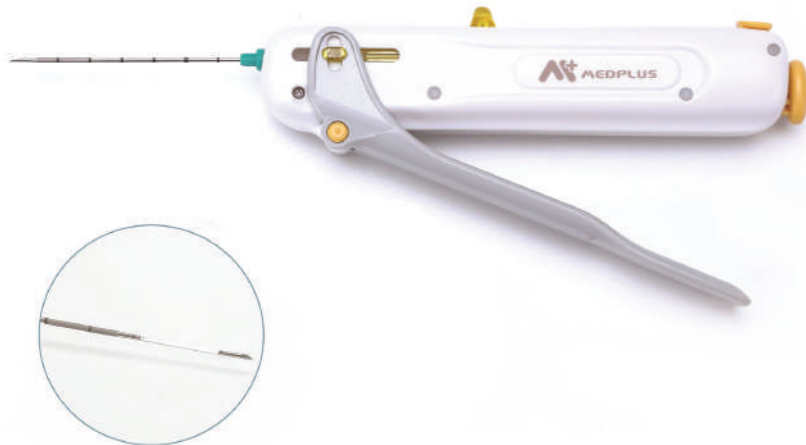


SEMI AUTOMATIC BIOPSY SYSTEM



BRAIN SWAB

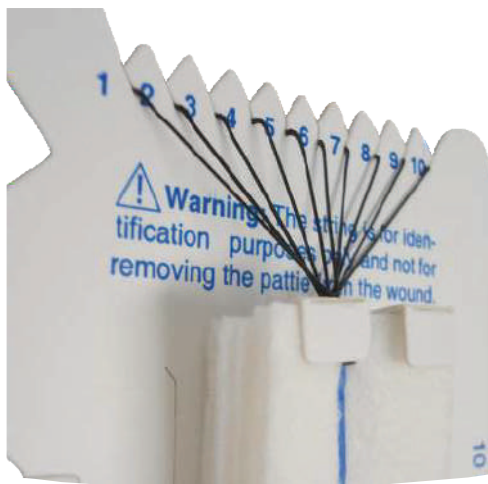

Standart Sizes

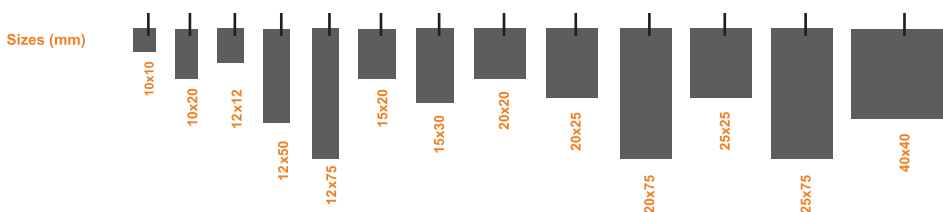

◆ ENDOBRONCHIAL TUBE

Endobronchial Tube

- Made of pvc in medical grade
- Available with left-sided and right-sided types
- The cuffs, two lumens and pilot balloons are imprinted with tracheal (clear) or bronchial (blue) for easy identification
- Smooth inner lumens allow easy passage of bronchoscopes
- Pre-loaded with stylet to help tube maintain shape for easier intubation
- Packed with switch connector and two low friction suction catheters

■ Left Side

| Size (Fr) | Cat. No. (DEHP-FREE) |
|-----------|----------------------|
| 28Fr | A03A01281F |
| 32Fr | A03A01321F |
| 35Fr | A03A01351F |
| 37Fr | A03A01371F |
| 39Fr | A03A01391F |
| 41Fr | A03A01411F |

■ Right Side

| Size (Fr) | Cat. No. (DEHP-FREE) |
|-----------|----------------------|
| 28Fr | A03A02281F |
| 32Fr | A03A02321F |
| 35Fr | A03A02351F |
| 37Fr | A03A02371F |
| 39Fr | A03A02391F |



TRACHEAL TUBES

- Made of softer PVC material, reducing risk of trauma



■ Nasal Tracheal Tube with High Volume, Low Profile Cuff

| Size ID (mm) | Cat. No. (DEHP-FREE) |
|--------------|----------------------|
| 5.0 | A01C08501F |
| 5.5 | A01C08551F |
| 6.0 | A01C08601F |
| 6.5 | A01C08651F |
| 7.0 | A01C08701F |
| 7.5 | A01C08751F |
| 8.0 | A01C08801F |
| 8.5 | A01C08851F |
| 9.0 | A01C08901F |

- Softer material for reducing risk of trauma and nasal bleeding
- Gently rounded tip for atraumatic intubation
- Preformed tube fits well for the nasal anatomy



■ Standard Tracheal Tube with High Volume, Low Profile Cuff


| Size ID (mm) | Cat. No. Bull Nose Tip (DEHP-FREE) |
|--------------|------------------------------------|
| 5.0 | A01A21501F |
| 5.5 | A01A21551F |
| 6.0 | A01A21601F |
| 6.5 | A01A21651F |
| 7.0 | A01A21701F |
| 7.5 | A01A21751F |
| 8.0 | A01A21801F |
| 8.5 | A01A21851F |
| 9.0 | A01A21901F |



■ Standard Tracheal Tube, Uncuffed

| Size ID (mm) | Cat. No. Bull Nose Tip (DEHP-FREE) |
|--------------|------------------------------------|
| 2.5 | A01A22253F |
| 3.0 | A01A22303F |
| 3.5 | A01A22353F |
| 4.0 | A01A22403F |
| 4.5 | A01A22453F |
| 5.0 | A01A22503F |
| 5.5 | A01A22553F |
| 6.0 | A01A22603F |
| 6.5 | A01A22653F |
| 7.0 | A01A22703F |
| 7.5 | A01A22753F |
| 8.0 | A01A22803F |
| 8.5 | A01A22853F |
| 9.0 | A01A22903F |


DISPOSABLE ENDOSCOPIC LINEAR CUTTER STAPLER AND CARTRIDGE

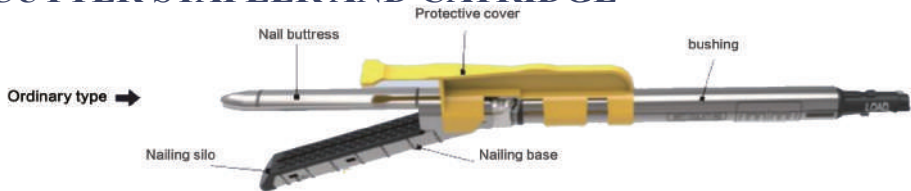

Properties and advantages of product innovation:

1. Gecko claw type design, enhances the clamping strength to tissue and greatly reduces the tissue movement.
2. With unequal staple height design, the reloads can accelerate the tissue recovery and improve the surgery efficiency.
3. "Water drop type" design in staple buttress provides better clinical "B" shape staple formation.

◆ Staple formation display



GIA-Stapler



Tri GST-Stapler



Water drop type

GASTROSTOMY TUBE

The gastrostomy tube provides outstanding product features for patient safety, comfort and ease of use for the patient or healthcare professional.

- ENFit connectors according to EN ISO80369-3 to avoid tubing misconnections with other systems. The G-Tube is available in single port and Y port.

- Maximum patient comfort due to soft, flexible high-quality medical grade silicone.

- Soft and adjustable retention plate for secure fixation. The structure of the retention plate achieves superior air circulation at the stoma site.

- Distance markings of 2cm

- Radiopaque stripe along the shaft


- High balloon stability of the inner retention balloon for long usage and secure fixation.

- Flat rounded tip allows for atraumatic insertion.

- Inflation port for balloon filling. This is colour coded to signify FR size.

- Imprint of the balloon volume on the shaft

- Recessed tip to prevent trauma once the balloon is inflated.

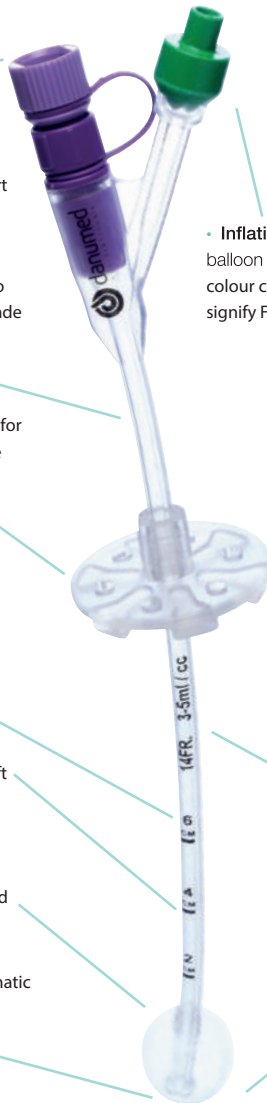

Reusable Silicone Standard Laryngeal Mask Airway

- Made of medical grade silicone, DEHP FREE & LATEX FREE.

| REF | Size | Patient Weight | Cuff Volume |
|----------|------|----------------|-------------|
| PA010310 | 1.0# | < 5kg | < 4ml |
| PA010315 | 1.5# | 5-10kg | < 7ml |
| PA010320 | 2.0# | 10-20kg | < 10ml |
| PA010325 | 2.5# | 20-30kg | < 14ml |
| PA010330 | 3.0# | 30-50kg | < 20ml |
| PA010340 | 4.0# | 50-70kg | < 30ml |
| PA010350 | 5.0# | 70-100kg | < 40ml |
| PA010360 | 6.0# | > 100kg | < 50ml |



Reusable Silicone Standard Laryngeal Mask Airway, with bar

- Made of medical grade silicone, DEHP FREE & LATEX FREE.

| REF | Size | Patient Weight | Cuff Volume |
|----------|------|----------------|-------------|
| PA011310 | 1.0# | < 5kg | < 4ml |
| PA011315 | 1.5# | 5-10kg | < 7ml |
| PA011320 | 2.0# | 10-20kg | < 10ml |
| PA011325 | 2.5# | 20-30kg | < 14ml |
| PA011330 | 3.0# | 30-50kg | < 20ml |
| PA011340 | 4.0# | 50-70kg | < 30ml |
| PA011350 | 5.0# | 70-100kg | < 40ml |



Reusable Silicone Reinforced Laryngeal Mask Airway

- Made of medical grade silicone, DEHP FREE & LATEX FREE.


| REF | Size | Patient Weight | Cuff Volume |
|----------|------|----------------|-------------|
| PA010410 | 1.0# | < 5kg | < 4ml |
| PA010415 | 1.5# | 5-10kg | < 7ml |
| PA010420 | 2.0# | 10-20kg | < 10ml |
| PA010425 | 2.5# | 20-30kg | < 14ml |
| PA010430 | 3.0# | 30-50kg | < 20ml |
| PA010440 | 4.0# | 50-70kg | < 30ml |
| PA010450 | 5.0# | 70-100kg | < 40ml |
| PA010460 | 6.0# | > 100kg | < 50ml |



Reusable Silicone Reinforced Laryngeal Mask Airway, with bar

- Made of medical grade silicone, DEHP FREE & LATEX FREE.

| REF | Size | Patient Weight | Cuff Volume |
|----------|------|----------------|-------------|
| PA011410 | 1.0# | < 5kg | < 4ml |
| PA011415 | 1.5# | 5-10kg | < 7ml |
| PA011420 | 2.0# | 10-20kg | < 10ml |
| PA011425 | 2.5# | 20-30kg | < 14ml |
| PA011430 | 3.0# | 30-50kg | < 20ml |
| PA011440 | 4.0# | 50-70kg | < 30ml |
| PA011450 | 5.0# | 70-100kg | < 40ml |



DUAL SEAL LARYNGEAL MASK WITH GASTRIC ACCESS (IGEL)

The dual seal laryngeal mask with gastric access aims to minimize the risk of aspiration and provide effective sealing with its dual seal design and gastric-access channel.


■ Features

- Gastric access channel for managing gastric content
- Stylet shapes anatomical curve, ensuring rapid and easy placement
- Medical grade silicone allows better biocompatibility
- Silicone cuff creates anatomical seal of the pharyngeal
- Disposable laryngeal mask reduces the risk of cross-contamination
- Pilot balloon shows mask size and provides tactile indication of inflation degree
- Bite block protects airway occlusion



| Mask Size | Patient Size | Largest Size of Gastric Tube | Cat. No. |
|-----------|--------------|------------------------------|------------|
| 1.5 | 5- 10kg | 10Fr | A05B021510 |
| 2 | 10-20kg | 10Fr | A05B022010 |
| 2.5 | 20-30kg | 14Fr | A05B022510 |
| 3 | 30-50kg | 16Fr | A05B023010 |
| 4 | 50-70kg | 16Fr | A05B024010 |
| 5 | 70-100kg | 18Fr | A05B025010 |

CENTRAL VENOUS CATHETER

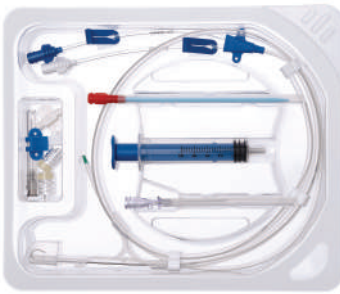

| Lumen Size | Size (Fr.) | Lumen Size (GA) | Length of indwelling Catheter (cm) | Extension line type | Flow rate ml/Min. |
|-----------------|------------|-----------------|------------------------------------|---------------------|-------------------|
| Triple Lumen | 7 Fr | 18 | 20 | Medial | 25 |
| | | 18 | | proximal | 27 |
| | | 16 | | Distal | 58 |
| | | 18 | | Medial | 22 |
| | 7 Fr | 18 | 30 | proximal | 23 |
| | | 16 | | Distal | 43 |
| | | 18 | | Medial | 15 |
| | | 18 | | proximal | 15 |
| Quadruple Lumen | 8FR | 16 | 16 | Distal | 64 |
| | | 18 | | Medial - 1 | 32 |
| | | 18 | | Medial - 2 | 31 |
| | | 18 | | Proximal | 31 |
| | 8FR | 16 | 20 | Distal | 57 |
| | | 18 | | Medial - 1 | 28 |
| | | 18 | | Medial - 2 | 29 |
| | | 18 | | Proximal | 27 |

DISPOSABLE APRON



| SIZE | WEIGHT | MATERIAL |
|-----------|--------|----------|
| 28" * 46" | 10G | PE |

TRACHEOSTOMY TUBE

- Tracheostomy Tube is a hollow tube, with or without a cuff, that is electively inserted directly into the trachea through a surgical incision or with a wire-guided progressive dilatation technique in case of an emergency.
- Lightweight tube made of Medical grade PVC for patient comfort. Full length Radio-opaque line for detection of correct placement. ISO standard connector for universal connection to ventilation equipment. Printed neck plate with size information for easy identification.
- Straps provided in the pack for fixation of the tube. Smooth rounded tip of the Obturator reduces trauma during insertion. Rigid blister pack provides maximum protection for the tube.

■ Cuffed

| Size ID (mm) | Cat. No. (DEHP-FREE) |
|--------------|----------------------|
| 3.0 | A02A05301F |
| 3.5 | A02A05351F |
| 4.0 | A02A05401F |
| 4.5 | A02A05451F |
| 5.0 | A02A05501F |
| 5.5 | A02A05551F |
| 6.0 | A02A05601F |
| 6.5 | A02A05651F |
| 7.0 | A02A05701F |
| 7.5 | A02A05751F |
| 8.0 | A02A05801F |
| 8.5 | A02A05851F |
| 9.0 | A02A05901F |
| 9.5 | A02A05951F |
| 10.0 | A02A05961F |



■ Uncuffed

| Size ID (mm) | Cat. No. (DEHP-FREE) |
|--------------|----------------------|
| 3.0 | A02A06303F |
| 3.5 | A02A06353F |
| 4.0 | A02A06403F |
| 4.5 | A02A06453F |
| 5.0 | A02A06503F |
| 5.5 | A02A06553F |
| 6.0 | A02A06603F |
| 6.5 | A02A06653F |
| 7.0 | A02A06703F |
| 7.5 | A02A06753F |
| 8.0 | A02A06803F |
| 8.5 | A02A06853F |
| 9.0 | A02A06903F |
| 9.5 | A02A06953F |
| 10.0 | A02A06963F |



■ SuctionPlus Tracheostomy Tube

| Size ID (mm) | Cat. No. (DEHP-FREE) |
|--------------|----------------------|
| 6.0 | A02C02601F |
| 6.5 | A02C02651F |
| 7.0 | A02C02701F |
| 7.5 | A02C02751F |
| 8.0 | A02C02801F |
| 8.5 | A02C02851F |
| 9.0 | A02C02901F |



Our Partners



Kampus Towers, Opp Central Police station, University way.
P.O. Box 2298 00200
Nairobi, Kenya.

MOBILE: +254 723 435 983/+254739534083/0771702356
EMAIL greatlab2015@gmail.com/info@greatlab.co.ke




No. **PVT-ZQUB572**

CERTIFICATE OF INCORPORATION

I hereby **CERTIFY** that,

GREAT LABORATORY & CHEMICAL SUPPLIERS LIMITED

is on this date 20 Jan 2021 Incorporated under the Companies Act, 2015 and that the Company is a **PRIVATE LIMITED COMPANY**.



.....
Registrar Of Companies

This is a system generated certificate. To validate this document send the word **BRS** to **21546**

www.kra.go.ke

Taxpayer PIN : P051984944V

Certificate Date: 18/02/2025

Name and Address :

GREAT LABORATORY & CHEMICAL SUPPLIERS LIMITED
CITY SQUARE, NAIROBI, Starehe District,
PO Box:2298,
Postal Code:00100

Certificate Number:

KRANON1455567225



**This is to confirm that GREAT LABORATORY &
CHEMICAL SUPPLIERS LIMITED,
Personal Identification Number P051984944V
has filed relevant tax returns and
paid taxes due as provided by Law.**

**This Certificate will be valid for
twelve (12) months up to 17/02/2026.**

Caveat: This certificate is issued on the basis of information available with the authority as at the certificate date mentioned above. The Authority reserves the right to withdraw the certificate if new evidence materially alters the tax compliance status of the recipient.

Disclaimer : This certificate is system Generated and therefore does not require signature. You may confirm validity of this certificate on the iTax Portal by using the TCC Checker. This certificate confirms your compliance status for a period of five years preceding the date of issue. The certificate may however be with withdrawn on grounds of outstanding debt affecting periods prior to this.

Certificate Date : 09/03/2023

Personal Identification Number

P051984944V

This is to certify that taxpayer shown herein has been registered with Kenya Revenue Authority

Taxpayer Information

| | |
|----------------------|---|
| Taxpayer Name | GREAT LABORATORY AND CHEMICAL SUPPLIERS LIMITED |
| Email Address | INFO@GREATLAB.CO.KE |

Registered Address

| | |
|-------------------------------------|------------------------------------|
| L.R. Number : | Building : CITY SQUARE |
| Street/Road : UNIVERSITY WAY | City/Town : NAIROBI |
| County : Nairobi | District : Starehe District |
| Tax Area : CBD | Station : North of Nairobi |
| P. O. Box : 2298 | Postal Code : 00100 |

Tax Obligation(s) Registration Details

| Sr. No. | Tax Obligation(s) | Effective From Date | Effective Till Date | Status |
|---------|-----------------------|---------------------|---------------------|--------|
| 1 | Value Added Tax (VAT) | 23/07/2022 | N.A. | Active |
| 2 | Income Tax - Company | 20/01/2021 | N.A. | Active |

The above PIN must appear on all your tax invoices and correspondences with Kenya Revenue Authority. Your accounting end month is December unless a change has been approved by the Commissioner-Domestic Taxes Department. The status of Tax Obligation(s) with 'Dormant' status will automatically change to 'Active' on date mentioned in "Effective Till Date" or any transaction done during the period. This certificate shall remain in force till further updated.

NT/PPD/2024/DGW/14960

VALID UNTIL: 09/12/2026



REPUBLIC OF KENYA

ACCESS TO GOVERNMENT PROCUREMENT OPPORTUNITIES (AGPO)

CERTIFICATE OF REGISTRATION

(WOMEN)

M/s GREAT LABORATORY & CHEMICAL SUPPLIERS LIMITED

Reg. No. PVT-ZQUB572

P. O. Box P.O BOX 2298 00

has on this 9TH day of DECEMBER, 2024,

been duly registered under The Public Procurement and Asset Disposal Act 2015 for a period of two years.



Disclaimer: You may confirm validity of this certificate on the AGPO Portal at www.agpo.go.ke or by scanning the QR Code provided.

Caveat: This certificate is issued on the basis of information available with the National Treasury as at the certificate date mentioned above. The National Treasury reserves the right to withdraw the certificate if new evidence materially alters the compliance status of the recipient.



NAIROBI CITY COUNTY

City Hall Building,
City Hall Way,
Nairobi, Kenya

P.O. Box 30075-00100
Nairobi, Kenya
info@nairobi.go.ke

UNIFIED BUSINESS PERMIT

TRADE LICENCE

LICENSE NO.: **UBP126812**
VALIDITY: **ANNUAL**

EFFECTIVE DATE: **27 JAN, 2025**
EXPIRY DATE: **26 JAN, 2026**

Nairobi City County grants this Trade License to

BUSINESS NAME: **GREAT LABORATORY AND CHEMICAL SUPPLIERS LIMITED - -**

Registration details:

Registration No.: -
KRA PIN: **P051984944V**
Postal address:

Physical address:

Unit: -, Floor: **5TH, CAMPUS TOWERS,**
Plot: **2838/12, UNIVERSITY WAY, Nairobi Central,**
Starehe, Nairobi

To engage in the following activities/businesses/occupations:

100 GENERAL TRADERS SHOPS AND RETAIL SERVICES
Medium non food trader shop/Agency retail service: 3-5 employees/50-300sq.m
- Other Health and Personal Care Retailers

Having paid a license fee of **KES. 18,500.00 (EIGHTEEN THOUSAND FIVE HUNDRED SHILLINGS ONLY)**

| | | |
|-----|--------------|----------------|
| 100 | SBP | KES. 15,000.00 |
| 200 | FIRE | KES. 2,500.00 |
| 400 | PEST CONTROL | KES. 1,000.00 |

BUSINESS UNDER THIS PERMIT SHALL BE CONDUCTED AT THE ADDRESS AS INDICATED

DISCLAIMER

Issuance of this permit does not exempt the permit holder from compliance checks, inspections, top-ups or adherence to applicable laws. The Nairobi City County Trade Licensing Act 2019 Section 17(1) gives the Director the powers to suspend or cancel a permit in case of false information or non-compliance with the applicable laws.

Date of Issue: **27 Jan, 2025**

POWERED BY

By Order of:



E-Verify

Scan this QR Code to verify the authenticity of this document

Alternatively visit nairobiservices.go.ke/everify and type in the document number

UBP126812

— Let's Make Nairobi Work —
www.nairobi.go.ke



NAIROBI CITY COUNTY

City Hall Building,
City Hall Way,
Nairobi, Kenya

P.O. Box 30075-00100
Nairobi, Kenya
info@nairobi.go.ke

TERMS & CONDITIONS

This licence is issued under section 12 of the Act subject to the following terms and conditions: -

1. Compliance with the provisions of the Nairobi City County Trade Licensing Act and any other legislation relevant to the trade.
2. This licence is not transferable.
3. Where a business is carried on in or from more than one premise, the business carried on in or from each premise is deemed to be separated business and as such a separate license is required;
4. The licence holder must notify the Director of any changes in the nature of trade, directorship or ownership of the business, location of business or cessation of trade.
5. The licence is a Nairobi City County Government property and must be displayed in a conspicuous place within the business premises and the licence holder must produce the licence whenever an authorized officer requires him or her.
6. The owner of the business should not sell/display their goods outside their licensed premises.
7. A person who forges or alters a licence without authority commits an offence and shall be liable on conviction to a fine not exceeding Kenya shillings fifty thousand or to imprisonment for a term not exceeding three months, or both.
8. A person who fails or neglects to renew a licence as required and continues to operate the business or trade commits an offence and shall be liable on conviction to a fine not exceeding Kenya shillings fifty thousand or to imprisonment for a term not exceeding three months, or both.
9. Granting of this License does not legitimise any illegal activity including occupation of a county road reserve or any prohibited area.
10. Under this license, it shall be the duty of every occupier, or owner or agent of a house, or other premise to clean or cause to be cleaned ten meters radius around his or her house or other premises or any area otherwise in his or her control
11. The licence holder shall ensure that appropriate safety measures are in place to mitigate fire and other hazards.
12. The licensed business shall only be conducted in full compliance with National and County health and safety laws and regulations.
13. The licensed business shall submit to periodic inspections for compliance with applicable standards, regulations and laws.
14. The licence holder shall comply with any other condition or directive as shall be necessary for purposes of health, hygiene and safety.
15. Subject to compliance to provided signage dimensions, siting & location requirements as per Outdoor Advertising & Signages policy (2015), NCG Advertising Act (2018) & PLUPA (2019).

POWERED BY





BUSINESS REGISTRATION SERVICE
P. O. BOX 30031
NAIROBI
6 MAY 2025

To
ALFRED KIPKURUI
P.O. Box 2298
00200 - CITY SQUARE

THE COMPANIES ACT, 2015

Records relating to the below company held by the Companies Registry as at **6 May 2025**

| | |
|---|---|
| COMPANY | GREAT LABORATORY & CHEMICAL SUPPLIERS LIMITED |
| COMPANY NUMBER | PVT-ZQUB572 |
| NOMINAL SHARE CAPITAL | 100,000.00 |
| NUMBER AND TYPE OF SHARES (VALUE PER SHARE) | ORDINARY: 100 (KES 1,000.00 EACH) |
| DATE OF REGISTRATION | 20TH JAN, 2021 |
| REGISTERED OFFICE | P.O BOX 2298 CITY SQUARE TELEPHONE: +254720449219, EMAIL: GREATLABKENYA@GMAIL.COM COUNTY: NAIROBI, DISTRICT: NAIROBI NORTH DISTRICT , LOCALITY: NAIROBI NORTH STREET: UNIVERSITY WAY, BUILDING: DELTA TOWERS |
| POSTAL ADDRESS | P.O BOX 2298 CITY SQUARE |
| ENCUMBRANCES | |

Name of Directors and Shareholders of the above company with their particular are as follows

| NAME | DESCRIPTION | ADDRESS | NATIONALITY | SHARES |
|------------------------------|----------------------|-------------------------------|-------------|-----------------|
| JOYCE JEBET KENEI | DIRECTOR/SHAREHOLDER | P.O BOX 9730 G.P.O NAIROBI | KENYAN | ORDINARY: 60 |
| MAUREEN JEROP KENEI KIBET | DIRECTOR/SHAREHOLDER | P.O BOX 9730 G.P.O NAIROBI | KENYAN | ORDINARY: 39 |
| MARGRET MUTHONI OGORO | DIRECTOR/SHAREHOLDER | P.O BOX 9730 G.P.O NAIROBI | KENYAN | ORDINARY: 1 |
| | | | TOTAL | 100 |

Yours Faithfully,
REGISTRAR OF COMPANIES



REF NO: OS-MDF2JE72

DISCLAIMER: THIS IS A SYSTEM GENERATED CERTIFICATE AND DOES NOT REQUIRE A SIGNATURE